This Page Is Inserted by IFW Operations and is not a part of the Official Record

BEST AVAILABLE IMAGES


Defective images within this document are accurate representations of the original documents submitted by the applicant.

Defects in the images may include (but are not limited to):


- BLACK BORDERS
- TEXT CUT OFF AT TOP, BOTTOM OR SIDES
- FADED TEXT
- ILLEGIBLE TEXT
- SKEWED/SLANTED IMAGES
- COLORED PHOTOS
- BLACK OR VERY BLACK AND WHITE DARK PHOTOS
- GRAY SCALE DOCUMENTS


IMAGES ARE BEST AVAILABLE COPY.


As rescanning documents will not correct images, please do not report the images to the Image Problem Mailbox.

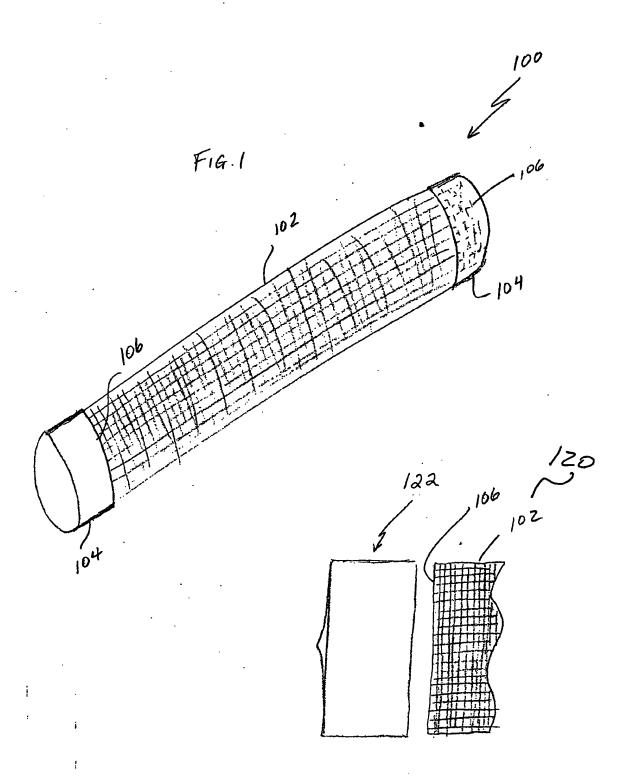

F16.2

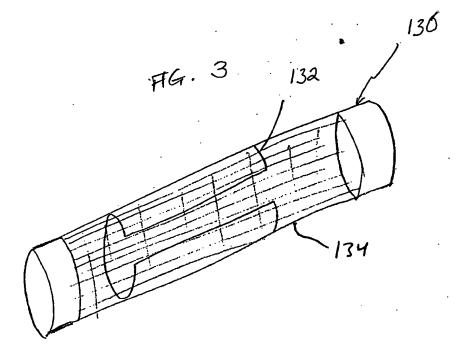


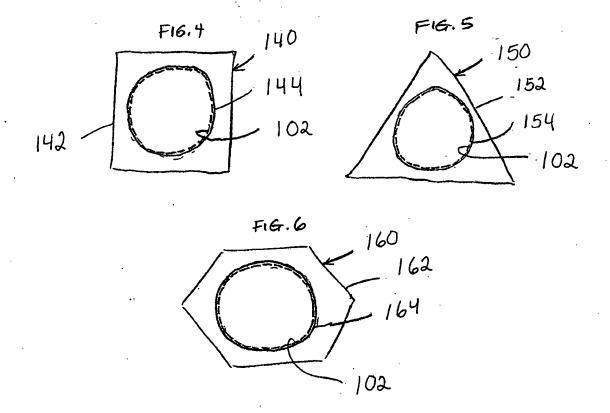


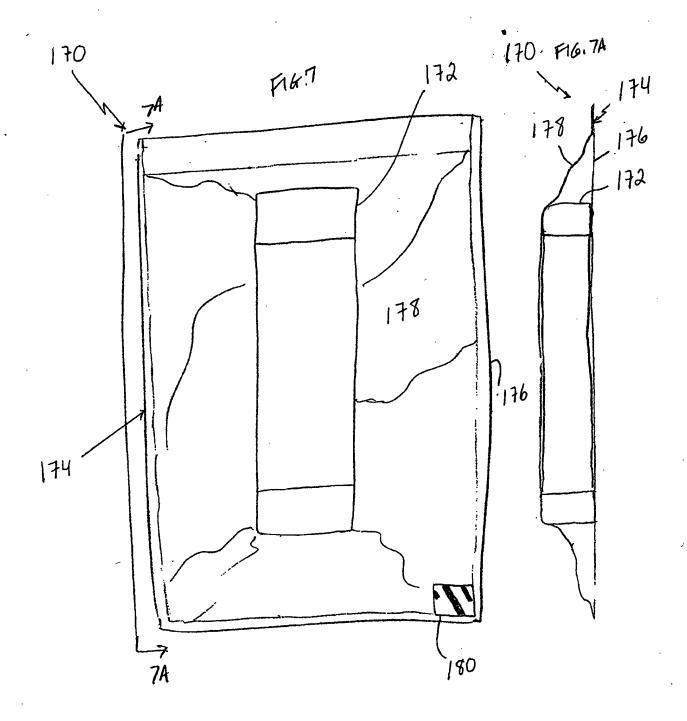

.

202	Provide a tube in a sterilized package at a point of use
	4
204_	Open the pockage
	1
Dolo	Remove the tube from the package
l	4
208 -	Remove the end cap from one end of tube
ڪ اه ــ	Place the used device in the tube
	The state of the s
212-	Replace the end cap on the tube
	<u> </u>
214	Remove the used devices in the tube from the point of use
214	- Place the tube containing the dovices in a both FIG 84
-	FIG 84

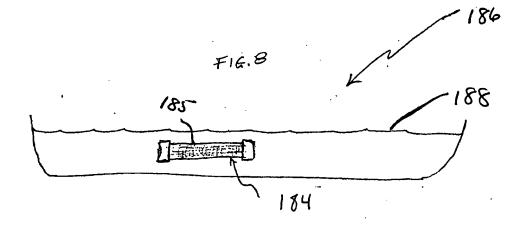

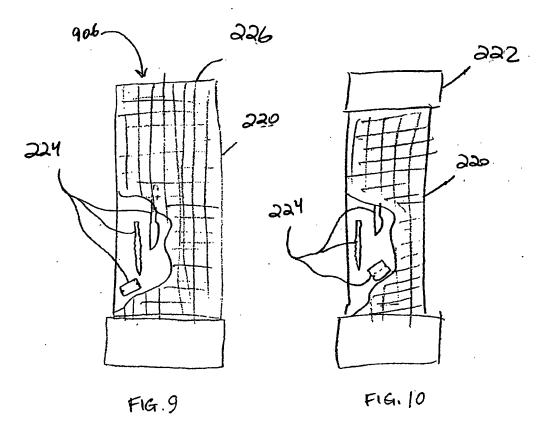




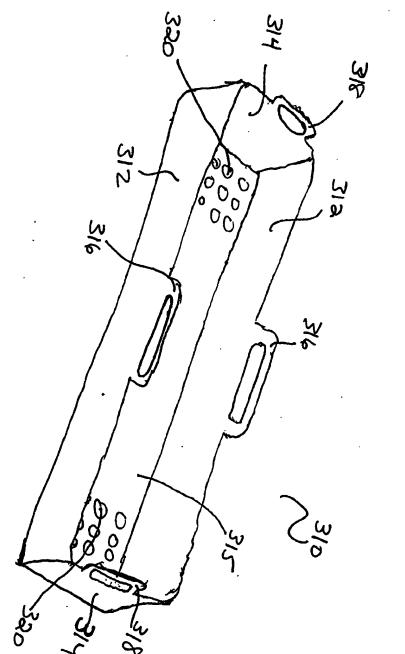



FIG. 1

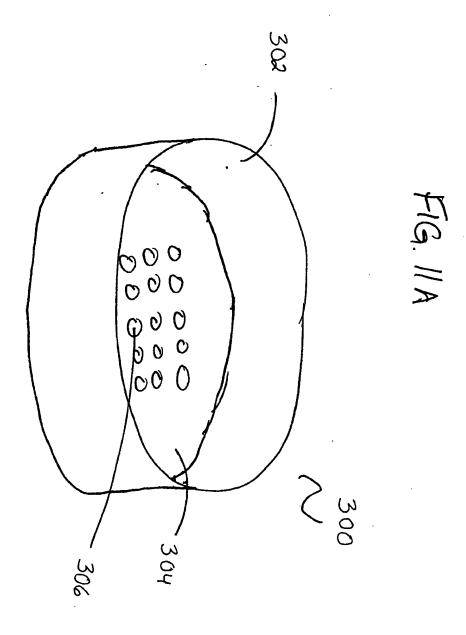


.

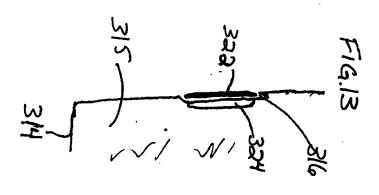


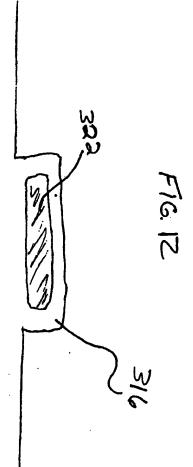


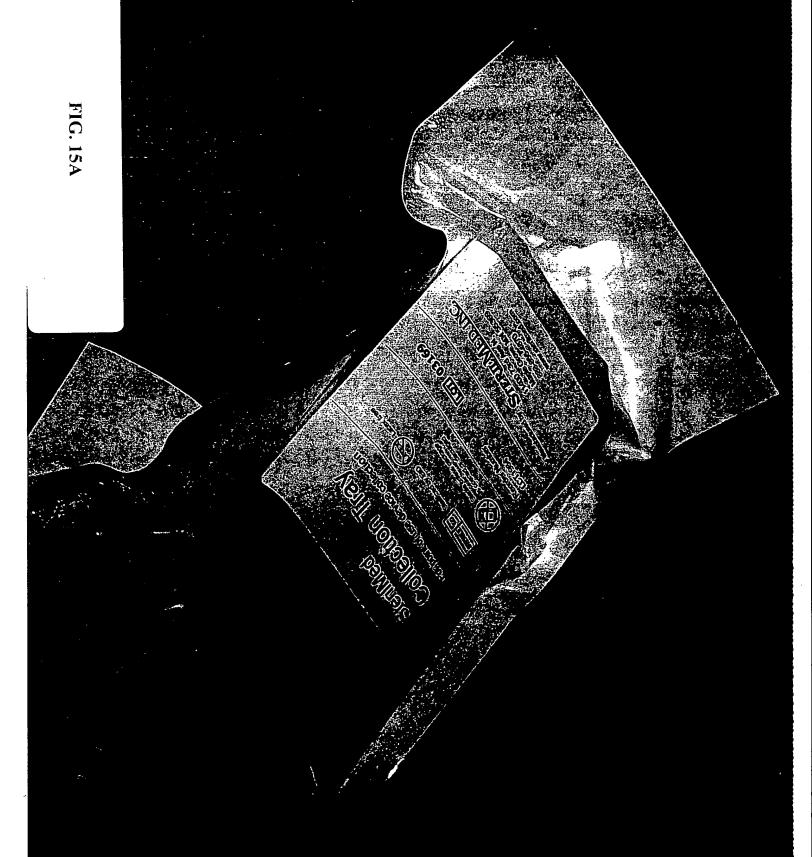


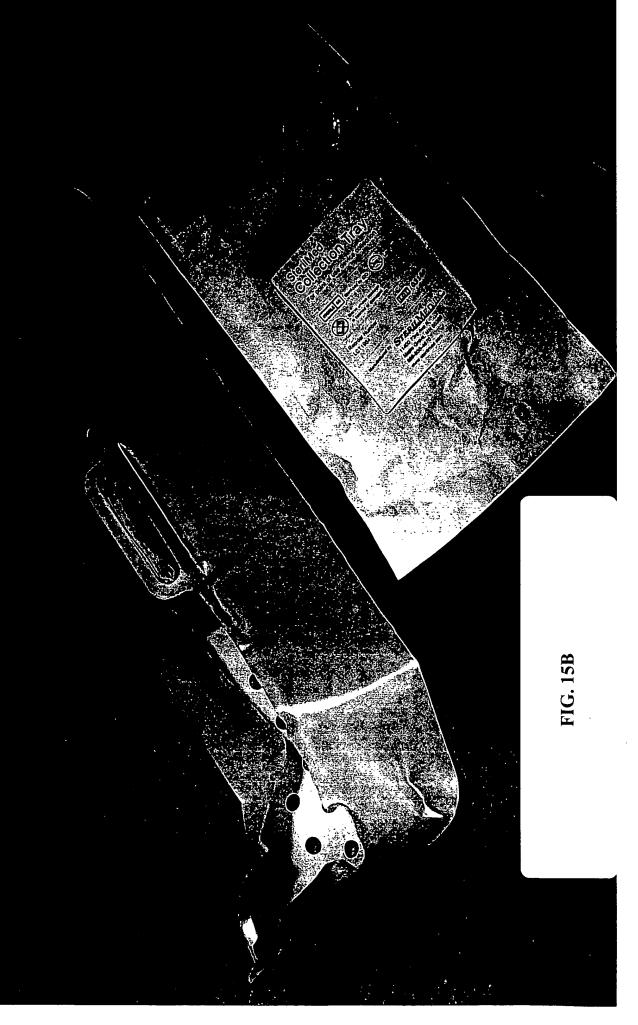

Collection Tray

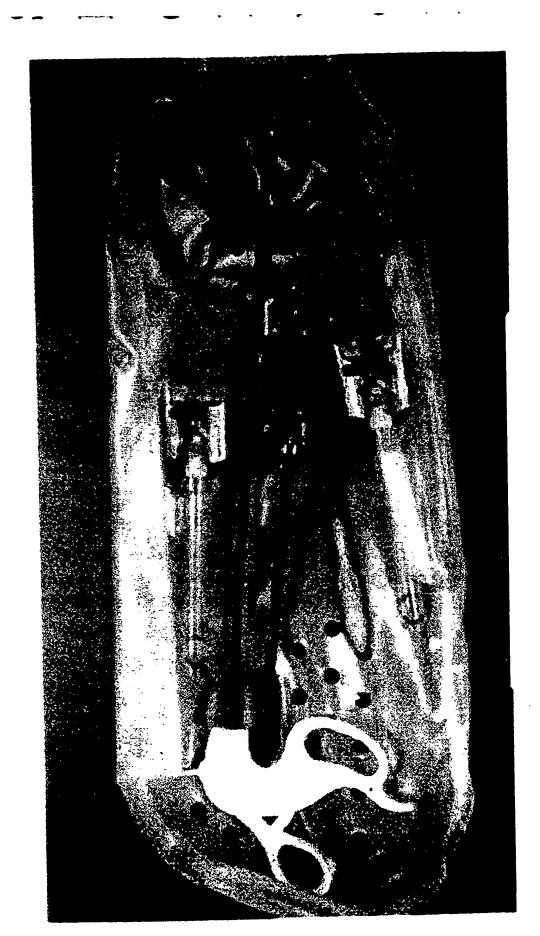

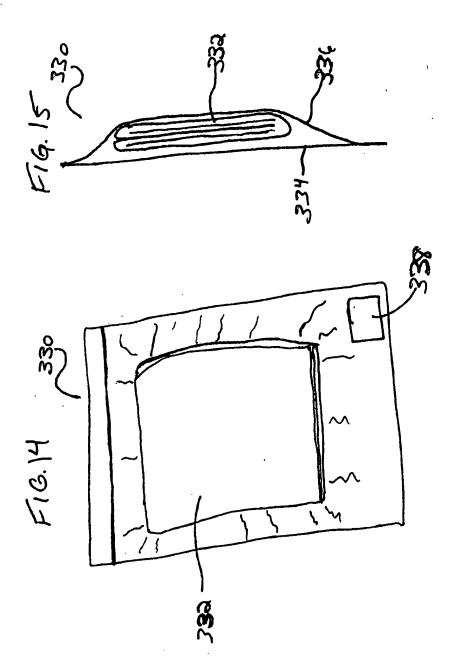

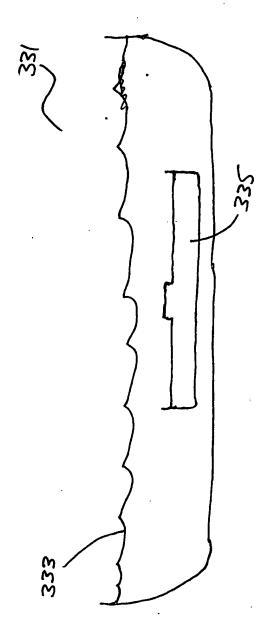

F19. 16A

